Power Electronics Measurement

In a world that loves pictures, why does real-time sampling and computation remain the best technique?

	Vrange: 300V PH1	POWER Arange: 10A total	fundamental	
	watts	1.3931kW	1.3911kW	
	VA VAr pf	1.6678kVA -917.08VAr 0.8353	1.4389kVA - 360.31VAr + 0.9668	
~~~	voltage	208.50V	179.88V	+000.00°
	current frequency	7.9991A 46.801Hz	7.9989A	-014.81°
	mechanical	1.0940kW 8.6953Nm	1.2014krp <i>m</i>	
	V ph-ph	8.6953Nm 420.60V	1.2014ki pm 351.43V	-330.02°

PPA5500

 Cal Power

 Via Acquanera, 29
 22100 COM0

Via Acquanera, 29 22100 tel. 031.526.566 (r.a.) fax 03 info@calpower.it www.ca

fax 031.507.984

N4L

#### Introduction

Most people reading this document will be directly or indirectly interested in the analysis of electrical power conversion and ultimately, in quantifying the power efficiency associated with a product or system.

Given the largely digital nature of modern measurement instrumentation, it is common for an engineer tasked with selection of a measurement instrument, to focus their efforts on the easily defined and commonly understood digital criteria of 'sample rate' or 'bit count' defined for a product of interest.

This focus is encouraged by many instrumentation manufacturers who benefit from such a simplistic approach, overlooking more complex and demanding considerations that usually make the specification of an A/D a largely meaningless criteria on which to select a precision power measurement instrument.

The primary challenge for precision measurement in power electronics is always the analogue hardware, including signal conditioning, data handling and ultimately calibration since it is these factors not the specification of an A/D device, that absolutely dominate measurement accuracy.

In this document, we consider misconceptions related to digital instrumentation and the functional elements of good design that dictate the total performance of all high-performance power measurement instruments.


#### Misconceptions - What's in a picture?

On the leading page of this document, the main picture shows a PPA5500 series power analyzer in front of a dual motor test system to which is it is connected.

The PPA is set in SCOPE mode as shown here, where a PWM voltage on one phase is visible, above the associated phase current.

We know from experience that:

- A. Users like to look at a picture and
- B. They assume that the same data points are used to derive quantitative measurements

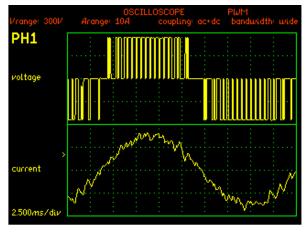



#### True real time computation architecture

For important reasons that we will explain in this document, the sampling and computation technique used in a PPA when in power analyzer (measurement) mode is completely different to that of the scope mode or indeed any conventional sampling design.

This results in an accuracy of measured values presented in the PPA Power Analyzer mode that is not achieved with a digital oscilloscope, DAQ or typical power analyzer.


In the following pages, we explain why.

Vrange: 300V	POWER Arange: 10A	ANALYZER coupling: ac+dc	PWM 14:55:52 bandwidth: wide
PH1	total	fundamental	
watts	1.3931kW	1.3930kW	
VA	1.6678kVA	1.4389kVA	
VAc	- 917.08VAr	-360.31VAr	
pf	0.8353	+0.9681	
voltage	208.50V	179.881/	+000.00°
current	7.9991A	7.9989A	-014.50°
frequency	46.803Hz		
mechanical	1.0940k₩		
	8.6953Nm	1.2014krpm	
V ph-ph	420.60V	351.431/	-330.02°

Power Measurement Techniques	© Newtons4th Ltd. 2022	Mar	⁻ 2022	Doc ref: D000625_2	Page <b>2</b> of <b>6</b>
Newtons4th Ltd 1	Bede Island Road Leicester	LE2 7EA	UK Tel	: +44 (0)116 2301066	

# **Conventional digitising techniques**

Oscilloscope and DAQ designs are primarily focused on a sampling speed and resolution that will suit a wide range of measurement applications and combine this variable sampling with memory, into which the derived samples can be stored or buffered.

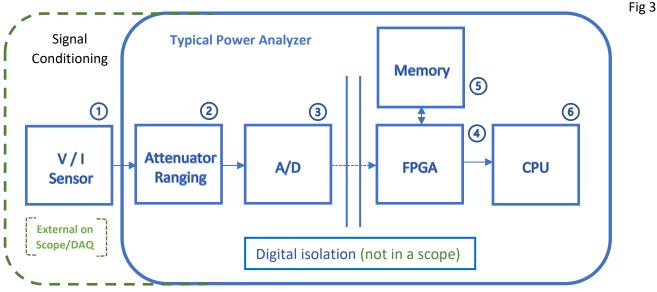


Key points relating to power analysis:

- Signal conditioning is often external, with measurement accuracy uncertainty that dominates total error
- Finite memory inevitably dictates the sample rate available as the time base is reduced
- Graphical presentation and measurements derived from time-based sample windows are asynchronous with primary power components and therefore require <u>averaging to achieve stability</u>

# Power analysis with Real Time sampling and computation

The PPA series incorporates signal conditioning specifically designed for the challenges of modern power applications and will therefore not suffer the measurement uncertainties associated with external devices. Additionally, and unique to the PPA analyzers, is an isolation and digital processing technique that removes the obstacle of digital memory size or speed.

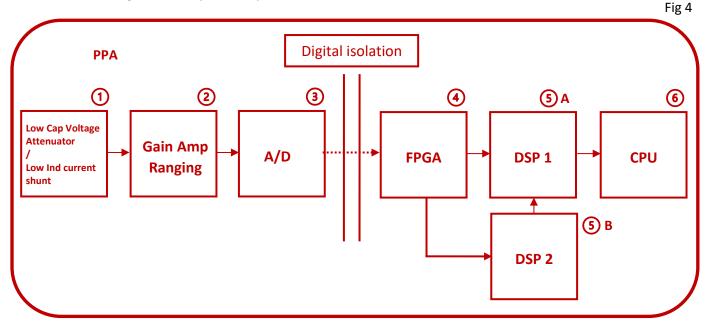


Power Measurement Techniques © Newtons4	:h Ltd. 2022 M	ar 2022	Doc ref: D000625_2	Page <b>3</b> of <b>6</b>
Newtons4th Ltd 1 Bede Island F	Road Leicester LE2 7EA	A UK Tel	: +44 (0)116 2301066	

# Precision Power Analysis – Deriving the right measurement values

Key points relating to power analysis:

- Proprietary voltage and current signal conditioning provide exceptionally flat response
- High frequency digital isolation eliminates signal uncertainty associated with conventional isolation
- Proprietary FPGA/DSP structure computes power real time at full sample rate irrespective of time base because there is no memory limitation
- Unique end to end calibration over the complete operating range provides market leading accuracy

#### Analogue and processing differentiators

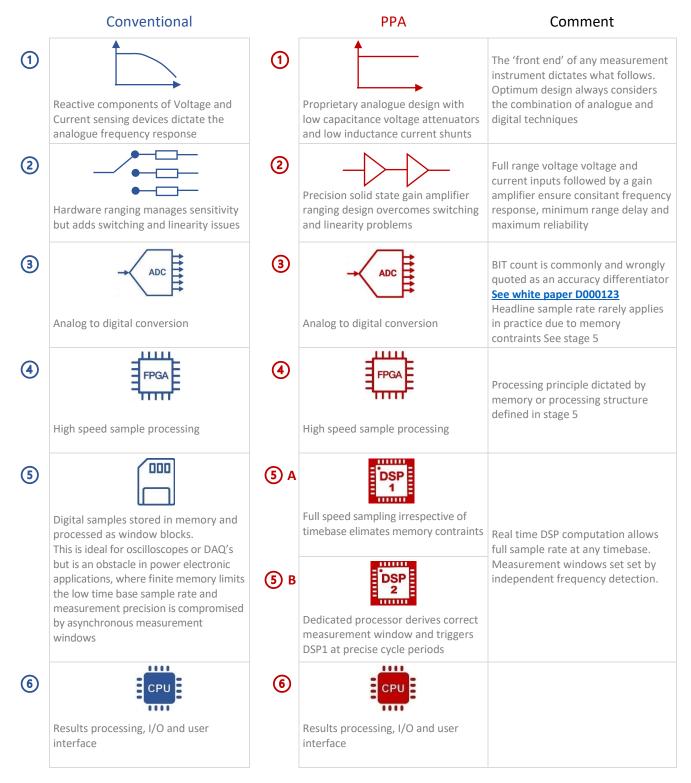

Power Measurement Techniqu	es © Newtons4th Ltd. 2022	Mar 2022	Doc ref: D000625_2	Page <b>4</b> of <b>6</b>
Newtons4th Ltd	1 Bede Island Road Leicester L	.E2 7EA UK Te	l: +44 (0)116 2301066	

# Avoiding memory constraints

In the world of oscilloscope and DAQ designs, the ability of a measurement instrument largely depends on memory, because this dictates the resolution of graphic presentation and measured values.

This conventional digitizing technique is not ideal in the field of modern AC power electronics, both because analysis is based upon finite memory size which limits the sample rate at low frequency, and because typical measurement windows are unlikely to be synchronous with a waveform of changing frequency.

# Scope / Memory based sampling

This is illustrated in the scope image from Fig 1, where a 2.5ms/div time base provides sample window (image) of just over one cycle.

With any oscilloscope or equivalent sampling technique, measurement windows are unlikely to equal a single cycle or an integer number of cycles, therefore measurements made from this same data will inevitably include windowing error. The same problem occurs in systems with no buffer that are sometimes called "fixed windowing" or "fixed update rate", because these processes are not sufficiently dynamic.


# **Real time sampling and computation**

In Fig 2, real time measurements are displayed using a higher sample rate than an equivalent scope mode and DPS2 (ref. P4) ensures real time synchronisation with the fundamental frequency.

Given the correct frequency, the PPA also makes DFT computation of all fundamental power components for the same measurement window


# Memory window (or fixed window) measurement versus Real Time computation

Asynchronous measurement windows will inevitably give an RMS value that is not equal to one cycle of an AC waveform under test. In this case, a correct value can only be obtained by averaging many windows.

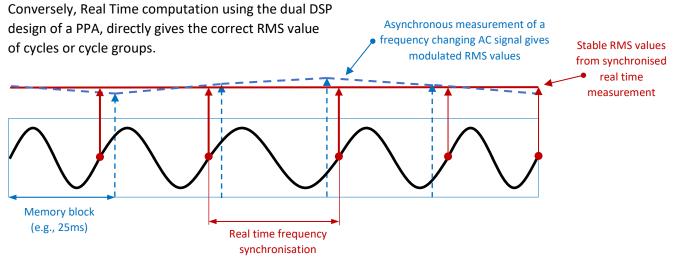

# The subject of sample windows and asynchronous measurements is discussed in White paper D000120

Power Measurement Techniques © Newtons4th Ltd. 2022	Mar 2022	Doc ref: D000625_2	Page <b>5</b> of <b>6</b>
Newtons4th Ltd 1 Bede Island Road Leicester L	.E2 7EA UK Tel	: +44 (0)116 2301066	






#### Presentation of data – Numbers and Images

CONTROL	Display PPA1	PPA2	Harmonics	PPAd	Capture	SETTIN	GS REA	AD PPA SET U	ar
CONTROL		- Arre	1110		uration: Acquisition Co			10.11M	wi
ACQU		OUPLING	RANGE		Wiring	3 Phase 3 Wat	itmeter 🗸	Frequency Reference	VVI
		APP		Speed		ed Medium ~		Phase Angle reference	m
ALARM		REMOTE	AUX	÷	Smoothing	Normal	~	Frequency Filte	an
					Smoothing Response	Auto-reset	~	Low Frequency	an
SY5		MODE	PROG		Frequency Reference	Voltage	~		со
Settings View		Control		ontrol		Software	of		
MULT	LOG	REAL TI	ME GRA	PH	LOG	STOP	CLEAR LOG	Instrument     Freeze Display	01
	- RESI	JLTS ncy Ph	41	V	Vatts PH1		W/a	tts PH2	
4.50	- 10 - 10 - 10 - 10 - 10 - 10 - 10 - 10	89 Hz	10000		1.276 W		5147,075	285 W	
		Itage F		_	Voltage F	PH2 F		oltage PH3	R
		.12 V			230.12 V			0.11 V	
RM		rrent F	PH2	100	Current F	НЗ	200		
	-	96 m/			90.93 mA	1000			

Having established that an instrument with real time sampling and computation can directly obtain power measurement values with the greatest speed and precision, a user will usually want measurements to be stored in a PC for convenient presentation and analysis. PPALoG PC software offered as a free download will communicate with up to 4 PPA instruments, to give real time log of up to 24 power phases plus analogue I/O signals.

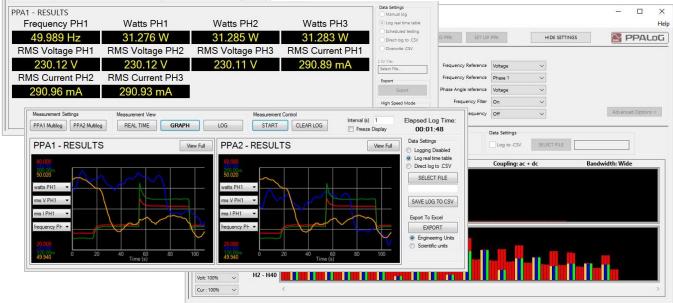

# Why is post processing of raw data not the ideal solution?

The appeal of processing raw data points in programs like MATLAB is clear and it is quite common for N4L to be asked if we support the direct transfer of samples made available to the FPGA of PPA series power analyzers, directly to a PC.

In the case of single shot raw data sample block, the answer is yes, but this is time and sample speed limited. The PPA architecture enables our instruments to provide directly computed values of all primary power parameters, derived from a gapless high speed sample rate and real time frequency synchronisation that is not possible via a communication port and external PC program.

So, while the raw data sample block is a useful feature for the post-capture analysis of a transient event, the architecture of the PPA provides direct and traceable measurement of power parameters that is usually the ultimate objective of external sample computation anyway.

# Conclusions

- Digital sampling techniques commonly used in Oscilloscopes / DAQ's while ideal for visual inspection and development, are not ideal for precision power analysis.
- Modern power applications represent both analogue and digital challenges not easily met by conventional digital sampling instruments.
- Post processing is suitable for transient analysis but not continuous power measurement
- Separate instruments are the ideal and usually the most economical solution, where quantitative measurement is via a Power Analyzer, and transient or visual analysis is via an Oscilloscope.
- <u>PC software</u> is the best solution for power measurement presentation and storage.

 Power Measurement Techniques © Newtons4th Ltd. 2022
 Mar 2022
 Doc ref: D000625_2
 Page 6 of 6

 Newtons4th Ltd
 1 Bede Island Road Leicester
 LE2 7EA
 UK
 Tel: +44 (0)116 2301066